



PROTECT YOUR PATIENT

THE DISKCOVER™ SYSTEM

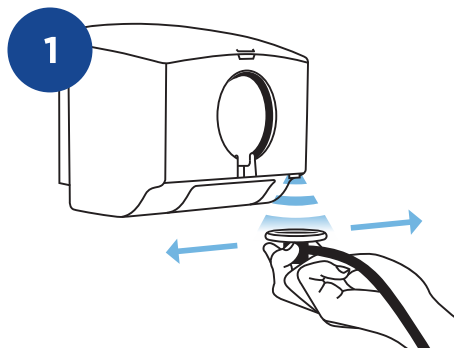


WAVE

Wave under touch-free sensor

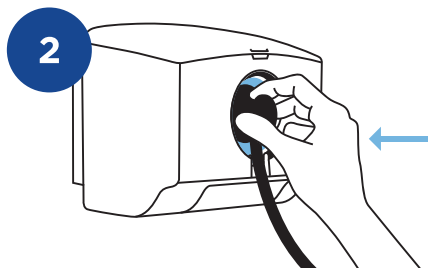

APPLY

Press firmly after light ring turns green



REMOVE

Withdraw with disk cover applied



For additional instructions, see inside dispenser lid
Questions? Call 1-844-980-2998 | DiskCover.com

© 2020 AseptiScope, Inc. All rights reserved. All trademarks referenced are trademarks of either AseptiScope or their respective owners. LBL-1005-00

REF | DSA-L1

PROTECT YOUR PATIENT


THE DISKCOVER™ SYSTEM

STETHOSCOPE COMPARISON

100%
Culture
Negative¹

An **ASEPTIC COVER** for
stethoscope diaphragms

IMPERVIOUS to biohazards
and contaminants*

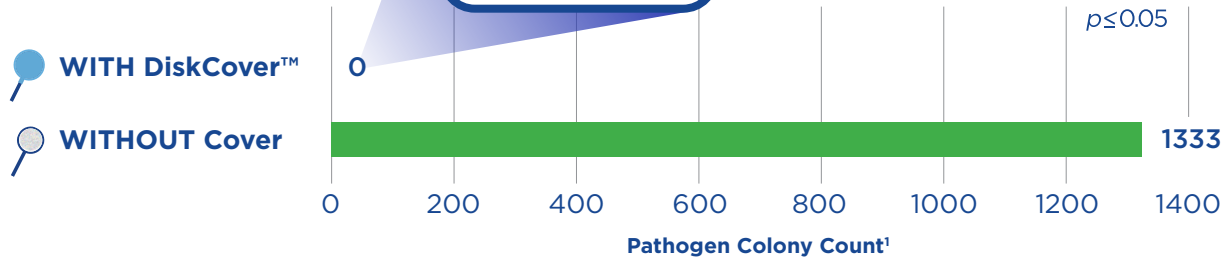

* Sputum, saliva, urine, feces, and superbugs, i.e., MRSA, CRE, C. Diff, VRE, E. Coli, etc.

¹Vasudevan R, et al. Mayo Clin Proc Innov Qual Outcomes. 2020;4(1):21-30.

**For additional instructions, see inside dispenser lid
Questions? Call 1-844-980-2998 | DiskCover.com**

© 2020 AseptiScope, Inc. All rights reserved. All trademarks referenced are trademarks of either AseptiScope or their respective owners. LBL-1006-00